

pipette dragon

[Top Pette Mechanical Pipettes (Adjustable & Fixed)]

All DRAGONLAB pipettes have been quality tested according to ISO8655-2:2002 with calibration certificate. The quality control involves gravimetric testing of each pipette with distilled water at 22°C.




Features for TopPette

- Lightweight, ergonomic, low force design
- Digital display clearly reads volume setting
- The pipettes cover volume range of 0.1µl to 10ml
- Easy to calibrate and maintain with tool supplied
- Design helps avoid repetitive strain injuries
- Calibrated in accordance with ISO8655. Each pipette supplied with individual test certificate
- The low part is available for autoclaving

Features for multi-channel TopPette

- 8 and 12 channel pipettes are available for standard 96-well plate
- Dispensing head rotates for optimum pipetting convenience
- Individual piston and tip cone assemblies allow easy repair and maintenance
- Compound material tip cone design allows visual seal verification
- Can be used with universal style pipette tips

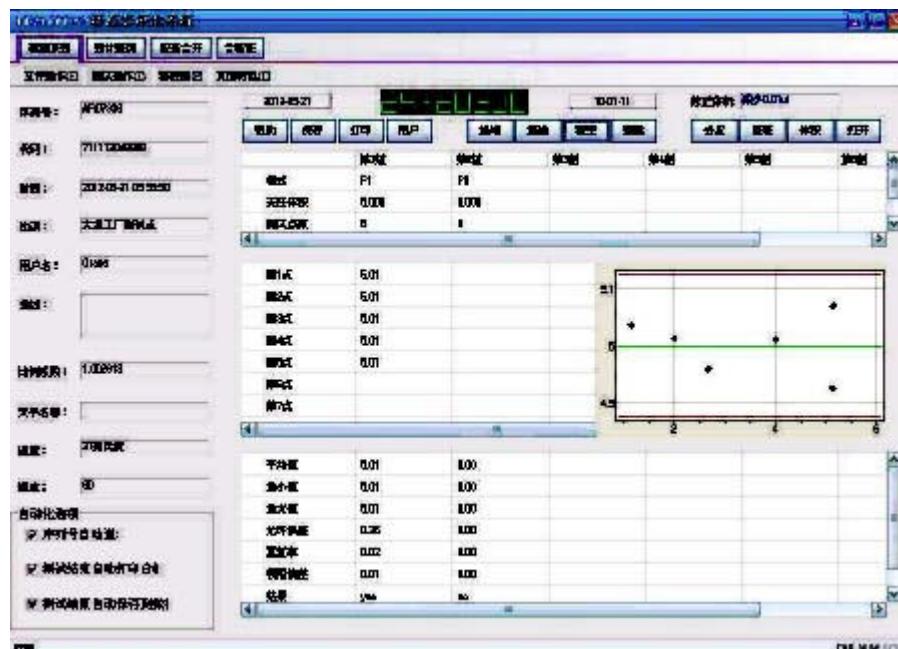

Calibration

Please visit our website for online calibration at www.dragon-lab.com. Through the online calibration software, users can perform simple, accurate and timely calibration with free cost, and avoid the calibration error due to non-professional operation.

We will support and help you to achieve consistently excellent results.

pipette dragon

Specifications

Single-channel Adjustable Volume Pipettes						
Volume Range	Increment	Test Volume	Maximum permissible systematic error (Inaccuracy)		Maximum permissible random error (Imprecision)	
			%	µL	%	µL
0.1-2.5µL	0.05µL	2.5µL	2.50%	0.0625	2.00%	0.05
		1.25µL	3.00%	0.0375	3.00%	0.0375
		0.25µL	12.00%	0.03	6.00%	0.015
0.5-10µL	0.1µL	10µL	1.00%	0.1	0.80%	0.08
		5µL	1.50%	0.075	1.50%	0.075
		1µL	2.50%	0.025	1.50%	0.015
2-20µL	0.5µL	20µL	0.90%	0.18	0.40%	0.08
		10µL	1.20%	0.12	1.00%	0.1
		2µL	3.00%	0.06	2.00%	0.04
5-50µL	0.5µL	50µL	0.60%	0.3	0.30%	0.15
		25µL	0.90%	0.225	0.60%	0.15
		5µL	2.00%	0.1	2.00%	0.1
10-100µL	1µL	100µL	0.80%	0.8	0.15%	0.15
		50µL	1.00%	0.5	0.40%	0.2
		10µL	3.00%	0.3	1.50%	0.15
20-200µL	1µL	200µL	0.60%	1.2	0.15%	0.3
		100µL	0.80%	0.8	0.30%	0.3
		20µL	3.00%	0.6	1.00%	0.2
50-200µL	1µL	200µL	0.60%	1.2	0.15%	0.3
		100µL	0.80%	0.8	0.30%	0.3
		50µL	1.00%	0.5	0.40%	0.2
100-1000µL	5µL	1000µL	0.60%	6	0.20%	2
		500µL	0.70%	3.5	0.25%	1.25
		100µL	2.00%	2	0.70%	0.7
200-1000µL	5µL	1000µL	0.60%	6	0.20%	2
		500µL	0.70%	3.5	0.25%	1.25
		200µL	0.90%	1.8	0.30%	0.6
1000-5000µL	50µL	5000µL	0.50%	25	0.15%	7.5
		2500µL	0.60%	15	0.30%	7.5
		1000µL	0.70%	7	0.30%	3
2-10mL	0.1mL	10mL	0.60%	60	0.20%	20
		5mL	1.20%	60	0.30%	15
		2mL	3.00%	60	0.60%	12

pipette dragon

8-channel Adjustable Volume Pipettes

Volume Range	Increment	Test Volume	Maximum permissible systematic error (Inaccuracy)		Maximum permissible random error (Imprecision)	
			%	µL	%	µL
0.5-10µL	0.1µL	10µL	1.50%	0.15	1.50%	0.15
		5µL	2.50%	0.125	2.50%	0.125
		1µL	4.00%	0.04	4.00%	0.04
5-50µL	0.5µL	50µL	1.00%	0.5	0.50%	0.25
		25µL	1.50%	0.375	1.00%	0.25
		5µL	3.00%	0.15	2.00%	0.1
50-300µL	5µL	300µL	0.70%	2.1	0.25%	0.75
		150µL	1.00%	1.5	0.50%	0.75
		50µL	1.50%	0.75	0.80%	0.4

12-channel Adjustable Volume Pipettes

Volume Range	Increment	Test Volume	Maximum permissible systematic error (Inaccuracy)		Maximum permissible random error (Imprecision)	
			%	µL	%	µL
0.5-10µL	0.1µL	10µL	1.50%	0.15	1.50%	0.15
		5µL	2.50%	0.125	2.50%	0.125
		1µL	4.00%	0.04	4.00%	0.04
5-50µL	0.5µL	50µL	1.00%	0.5	0.50%	0.25
		25µL	1.50%	0.375	1.00%	0.25
		5µL	3.00%	0.15	2.00%	0.1
50-300µL	5µL	300µL	0.70%	2.1	0.25%	0.75
		150µL	1.00%	1.5	0.50%	0.75
		50µL	1.50%	0.75	0.80%	0.4

Fixed Volume Pipettes

Volume Range	Increment	Test Volume	Maximum permissible systematic error (Inaccuracy)		Maximum permissible random error (Imprecision)	
			%	µL	%	µL
5µL	-	5µL	1.3%	0.065	1.2%	0.06
10µL	-	10µL	0.8%	0.08	0.8%	0.08
20µL	-	20µL	0.6%	0.12	0.5%	0.1
25µL	-	25µL	0.5%	0.125	0.3%	0.075
50µL	-	50µL	0.5%	0.25	0.3%	0.15
100µL	-	100µL	0.5%	0.5	0.3%	0.3
200µL	-	200µL	0.4%	0.8	0.2%	0.4
250µL	--	250µL	0.4%	1.0	0.2%	0.5
500µL	-	500µL	0.3%	1.5	0.2%	1.0
1000µL	-	1000µL	0.3%	3.0	0.2%	2.0
2000µL	-	2000µL	0.3%	6.0	0.15%	3.0
5000µL	-	5000µL	0.3%	15	0.15%	7.5

【MicroPette Mechanical Pipettes (Adjustable & Fixed)】

All DRAGONLAB pipettes have been quality tested according to ISO8655-2:2002 with calibration certificate. The quality control involves gravimetric testing of each pipette with distilled water at 22°C.


Features for MicroPette

- Lightweight, ergonomic, low force design
- Digital display clearly reads volume setting
- The pipettes cover volume range of 0.1µl to 10ml
- Easy to calibrate and maintain with tool supplied
- Design helps avoid repetitive strain injuries
- Calibrated in accordance with ISO8655. Each pipette supplied with individual test certificate
- The low part is available for autoclaving
- Manufactured from innovative materials



Features for multi-channel MicroPette

- 8 and 12 channel pipettes are available for standard 96-well plate
- Dispensing head rotates for optimum pipetting convenience
- Individual piston and tip cone assemblies allow easy repair and maintenance
- Compound material tip cone design allows visual seal verification
- Can be used with universal style pipette tips

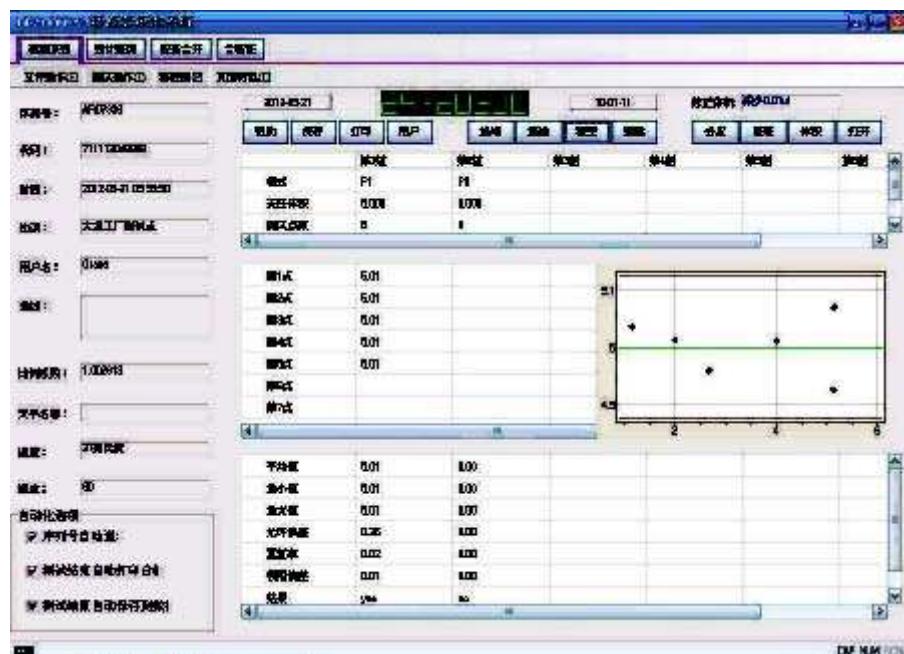

Calibration

Please visit our website for online calibration at www.dragon-lab.com. Through the online calibration software, users can perform simple, accurate and timely calibration with free cost, and avoid the calibration error due to non-professional operation.

We will support and help you to achieve consistently excellent results.

pipette dragon

Specifications

Single-channel Adjustable Volume Pipettes

Volume Range	Increment	Test Volume	Maximum permissible systematic error (Inaccuracy)		Maximum permissible random error (Imprecision)	
			%	µL	%	µL
0.1-2.5µL	0.05µL	2.5µL	2.50%	0.0625	2.00%	0.05
		1.25µL	3.00%	0.0375	3.00%	0.0375
		0.25µL	12.00%	0.03	6.00%	0.015
0.5-10µL	0.1µL	10µL	1.00%	0.1	0.80%	0.08
		5µL	1.50%	0.075	1.50%	0.075
		1µL	2.50%	0.025	1.50%	0.015
2-20µL	0.5µL	20µL	0.90%	0.18	0.40%	0.08
		10µL	1.20%	0.12	1.00%	0.1
		2µL	3.00%	0.06	2.00%	0.04
5-50µL	0.5µL	50µL	0.60%	0.3	0.30%	0.15
		25µL	0.90%	0.225	0.60%	0.15
		5µL	2.00%	0.1	2.00%	0.1
10-100µL	1µL	100µL	0.80%	0.8	0.15%	0.15
		50µL	1.00%	0.5	0.40%	0.2
		10µL	3.00%	0.3	1.50%	0.15
20-200µL	1µL	200µL	0.60%	1.2	0.15%	0.3
		100µL	0.80%	0.8	0.30%	0.3
		20µL	3.00%	0.6	1.00%	0.2
50-200µL	1µL	200µL	0.60%	1.2	0.15%	0.3
		100µL	0.80%	0.8	0.30%	0.3
		50µL	1.00%	0.5	0.40%	0.2
100-1000µL	5µL	1000µL	0.60%	6	0.20%	2
		500µL	0.70%	3.5	0.25%	1.25
		100µL	2.00%	2	0.70%	0.7
200-1000µL	5µL	1000µL	0.60%	6	0.20%	2
		500µL	0.70%	3.5	0.25%	1.25
		200µL	0.90%	1.8	0.30%	0.6
1000-5000µL	50µL	5000µL	0.50%	25	0.15%	7.5
		2500µL	0.60%	15	0.30%	7.5
		1000µL	0.70%	7	0.30%	3
2-10mL	0.1mL	10mL	0.60%	60	0.20%	20
		5mL	1.20%	60	0.30%	15
		2mL	3.00%	60	0.60%	12

8-channel Adjustable Volume Pipettes

Volume Range	Increment	Test Volume	Maximum permissible systematic error (Inaccuracy)		Maximum permissible random error (Imprecision)	
			%	µL	%	µL
0.5-10µL	0.1µL	10µL	1.50%	0.15	1.50%	0.15
		5µL	2.50%	0.125	2.50%	0.125
		1µL	4.00%	0.04	4.00%	0.04
5-50µL	0.5µL	50µL	1.00%	0.5	0.50%	0.25
		25µL	1.50%	0.375	1.00%	0.25
		5µL	3.00%	0.15	2.00%	0.1
50-300µL	5µL	300µL	0.70%	2.1	0.25%	0.75
		150µL	1.00%	1.5	0.50%	0.75
		50µL	1.50%	0.75	0.80%	0.4

12-channel Adjustable Volume Pipettes

Volume Range	Increment	Test Volume	Maximum permissible systematic error (Inaccuracy)		Maximum permissible random error (Imprecision)	
			%	µL	%	µL
0.5-10µL	0.1µL	10µL	1.50%	0.15	1.50%	0.15
		5µL	2.50%	0.125	2.50%	0.125
		1µL	4.00%	0.04	4.00%	0.04
5-50µL	0.5µL	50µL	1.00%	0.5	0.50%	0.25
		25µL	1.50%	0.375	1.00%	0.25
		5µL	3.00%	0.15	2.00%	0.1
50-300µL	5µL	300µL	0.70%	2.1	0.25%	0.75
		150µL	1.00%	1.5	0.50%	0.75
		50µL	1.50%	0.75	0.80%	0.4

Fixed Volume Pipettes

Volume Range	Increment	Test Volume	Maximum permissible systematic error (Inaccuracy)		Maximum permissible random error (Imprecision)	
			%	µL	%	µL
5µL	-	5µL	1.3%	0.065	1.2%	0.06
10µL	-	10µL	0.8%	0.08	0.8%	0.08
20µL	-	20µL	0.6%	0.12	0.5%	0.1
25µL	-	25µL	0.5%	0.125	0.3%	0.075
50µL	-	50µL	0.5%	0.25	0.3%	0.15
100µL	-	100µL	0.5%	0.5	0.3%	0.3
200µL	-	200µL	0.4%	0.8	0.2%	0.4
250µL	--	250µL	0.4%	1.0	0.2%	0.5
500µL	-	500µL	0.3%	1.5	0.2%	1.0
1000µL	-	1000µL	0.3%	3.0	0.2%	2.0
2000µL	-	2000µL	0.3%	6.0	0.15%	3.0
5000µL	-	5000µL	0.3%	15	0.15%	7.5

pipette dragon

【MicroPette Plus Autoclavable Pipette (Adjustable & Fixed)】

All DRAGONLAB pipettes have been quality tested according to ISO8655-2:2002 with calibration certificate. The quality control involves gravimetric testing of each pipette with distilled water at 22°C.

Fully autoclavable

The MicroPette plus pipettes can be fully autoclaved and withstood steam sterilizes at 121°C, 1 atm for 20 minutes. The pipettes can be autoclaved without special preparations. After autoclaving the pipette must be cooled down and left to dry over 12 hours. It is recommended to check the performance of the pipette after each autoclaving. It is also recommended to grease the piston and seal of the pipette after each 10 autoclaving.




Features for MicroPette plus

- Fully autoclavable
- Lightweight, ergonomic, low force design
- Digital display clearly reads volume setting
- The pipettes cover volume range of 0.1µl to 10ml
- Easy to calibrate and maintain with tool supplied
- Design helps avoid repetitive strain injuries
- Manufactured from innovative material
- Calibrated in accordance with ISO8655. Each pipette supplied with individual test certificate

Features for multi-channel MicroPette plus

- 8 and 12 channel pipettes are available for standard 96-well plate
- Dispensing head rotates for optimum pipetting convenience
- Individual piston and tip cone assemblies allow easy repair and maintenance
- Compound material tip cone design allows visual seal verification
- Can be used with universal style pipette tips

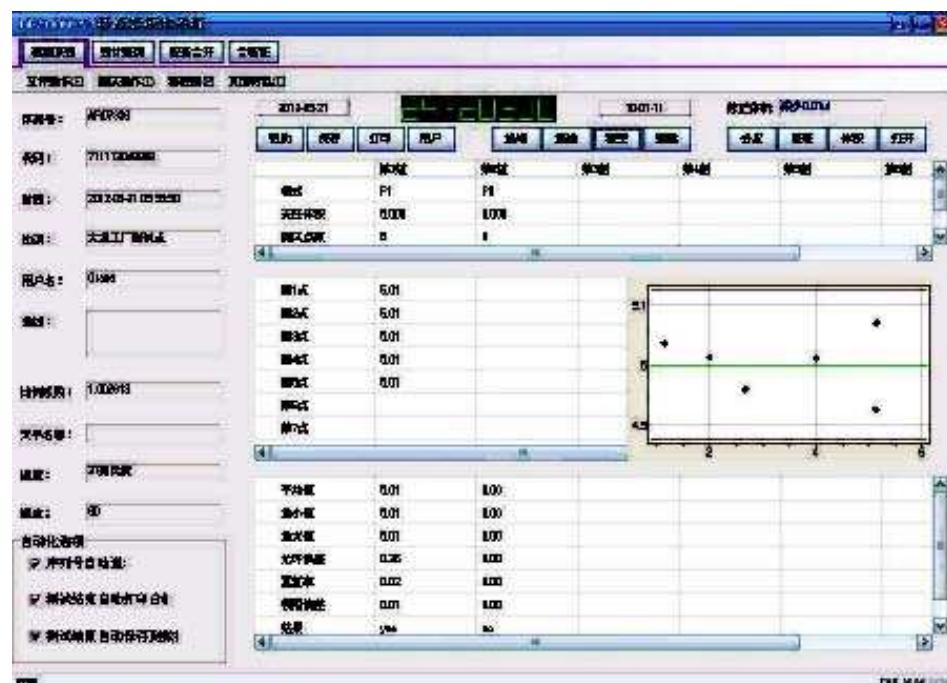

Calibration

Please visit our website for online calibration at www.dragon-lab.com. Through the online calibration software, users can perform simple, accurate and timely calibration with free cost, and avoid the calibration error due to non-professional operation.

We will support and help you to achieve consistently excellent results.

pipette dragon

pipette dragon

Specifications

Single-channel Adjustable Volume Pipettes					
Volume Range	Increment	Test Volume	Maximum permissible systematic error (Inaccuracy)		Maximum permissible random error (Imprecision)
			%	µL	
0.1-2.5µL	0.05µL	2.5µL	2.50%	0.0625	2.00% 0.05
		1.25µL	3.00%	0.0375	3.00% 0.0375
		0.25µL	12.00%	0.03	6.00% 0.015
0.5-10µL	0.1µL	10µL	1.00%	0.1	0.80% 0.08
		5µL	1.50%	0.075	1.50% 0.075
		1µL	2.50%	0.025	1.50% 0.015
2-20µL	0.5µL	20µL	0.90%	0.18	0.40% 0.08
		10µL	1.20%	0.12	1.00% 0.1
		2µL	3.00%	0.06	2.00% 0.04
5-50µL	0.5µL	50µL	0.60%	0.3	0.30% 0.15
		25µL	0.90%	0.225	0.60% 0.15
		5µL	2.00%	0.1	2.00% 0.1
10-100µL	1µL	100µL	0.80%	0.8	0.15% 0.15
		50µL	1.00%	0.5	0.40% 0.2
		10µL	3.00%	0.3	1.50% 0.15
20-200µL	1µL	200µL	0.60%	1.2	0.15% 0.3
		100µL	0.80%	0.8	0.30% 0.3
		20µL	3.00%	0.6	1.00% 0.2
50-200µL	1µL	200µL	0.60%	1.2	0.15% 0.3
		100µL	0.80%	0.8	0.30% 0.3
		50µL	1.00%	0.5	0.40% 0.2
100-1000µL	5µL	1000µL	0.60%	6	0.20% 2
		500µL	0.70%	3.5	0.25% 1.25
		100µL	2.00%	2	0.70% 0.7
200-1000µL	5µL	1000µL	0.60%	6	0.20% 2
		500µL	0.70%	3.5	0.25% 1.25
		200µL	0.90%	1.8	0.30% 0.6
1000-5000µL	50µL	5000µL	0.50%	25	0.15% 7.5
		2500µL	0.60%	15	0.30% 7.5
		1000µL	0.70%	7	0.30% 3
2-10mL	0.1mL	10mL	0.60%	60	0.20% 20
		5mL	1.20%	60	0.30% 15
		2mL	3.00%	60	0.60% 12

pipette dragon

8-channel Adjustable Volume Pipettes

Volume Range	Increment	Test Volume	Maximum permissible systematic error (Inaccuracy)		Maximum permissible random error (Imprecision)	
			%	µL	%	µL
0.5-10µL	0.1µL	10µL	1.50%	0.15	1.50%	0.15
		5µL	2.50%	0.125	2.50%	0.125
		1µL	4.00%	0.04	4.00%	0.04
5-50µL	0.5µL	50µL	1.00%	0.5	0.50%	0.25
		25µL	1.50%	0.375	1.00%	0.25
		5µL	3.00%	0.15	2.00%	0.1
50-300µL	5µL	300µL	0.70%	2.1	0.25%	0.75
		150µL	1.00%	1.5	0.50%	0.75
		50µL	1.50%	0.75	0.80%	0.4

12-channel Adjustable Volume Pipettes

Volume Range	Increment	Test Volume	Maximum permissible systematic error (Inaccuracy)		Maximum permissible random error (Imprecision)	
			%	µL	%	µL
0.5-10µL	0.1µL	10µL	1.50%	0.15	1.50%	0.15
		5µL	2.50%	0.125	2.50%	0.125
		1µL	4.00%	0.04	4.00%	0.04
5-50µL	0.5µL	50µL	1.00%	0.5	0.50%	0.25
		25µL	1.50%	0.375	1.00%	0.25
		5µL	3.00%	0.15	2.00%	0.1
50-300µL	5µL	300µL	0.70%	2.1	0.25%	0.75
		150µL	1.00%	1.5	0.50%	0.75
		50µL	1.50%	0.75	0.80%	0.4

Fixed Volume Pipettes

Volume Range	Increment	Test Volume	Maximum permissible systematic error (Inaccuracy)		Maximum permissible random error (Imprecision)	
			%	µL	%	µL
5µL	-	5µL	1.3%	0.065	1.2%	0.06
10µL	-	10µL	0.8%	0.08	0.8%	0.08
20µL	-	20µL	0.6%	0.12	0.5%	0.1
25µL	-	25µL	0.5%	0.125	0.3%	0.075
50µL	-	50µL	0.5%	0.25	0.3%	0.15
100µL	-	100µL	0.5%	0.5	0.3%	0.3
200µL	-	200µL	0.4%	0.8	0.2%	0.4
250µL	--	250µL	0.4%	1.0	0.2%	0.5
500µL	-	500µL	0.3%	1.5	0.2%	1.0
1000µL	-	1000µL	0.3%	3.0	0.2%	2.0
2000µL	-	2000µL	0.3%	6.0	0.15%	3.0
5000µL	-	5000µL	0.3%	15	0.15%	7.5